

## Optimization of GlycoWorks HILIC SPE for the Quantitative and Robust Recovery of N-Linked Glycans from mAb-Type Samples

Matthew A. Lauber, Stephan M. Koza, and Kenneth J. Fountain  
 Waters Corporation, Milford, MA, USA

### APPLICATION BENEFITS

- GlycoWorks HILIC  $\mu$ Elution Plate provides an efficient mechanism for glycan cleanup
- Quantitative and consistent recoveries for a diverse range of N-glycans with optimized SPE conditions
- Optimized SPE conditions also confer excellent method robustness
- Availability of a 2-AB labeled glycan standard for ensuring the performance of sample preparation and analysis methods

### WATERS SOLUTIONS

ACQUITY UPLC® H-Class Bio System

ACQUITY UPLC GST Amide  
 (BEH Glycan) Column

GlycoWorks™ 96-well HILIC  
 $\mu$ Elution Plate

Glycan Performance Test Standard

### KEY WORDS

N-glycans, GlycoWorks, BEH glycan,  
 Glycan Performance Test Standard, HILIC,  
 HILIC SPE

### INTRODUCTION

More than half of all proteins are estimated to be glycosylated.<sup>1,2</sup> This post-translational modification, involving the attachment of oligosaccharides, plays a very significant role in many biological processes.<sup>3</sup> Therapeutic antibodies are a salient example of a set of proteins affected by glycosylation, given that their efficacy and immunogenicity can be considerably attenuated by changes in their glycan profile. Glycan profiles of therapeutic antibodies are often, therefore, a critical quality attribute (CQA) that must be assessed during cell line selection and monitored during development and batch releases.

A highly effective analysis platform for evaluating N-glycans from glycoproteins involves the release of glycans by PNGase F, their labeling with fluorescently active 2-aminobenzamide (2-AB), subsequent separation by hydrophilic interaction chromatography (HILIC), and detection by fluorescence (FLR), as shown in Figure 1:<sup>3-10</sup>

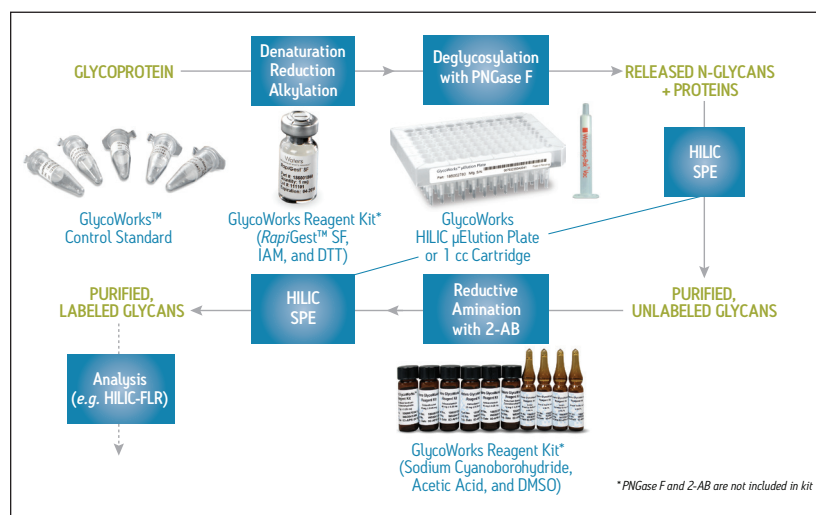


Figure 1. Schematic for preparing 2-AB labeled glycans from a glycoprotein using GlycoWorks. Consumables that are included as part of the GlycoWorks solution are highlighted in blue. Note that PNGase F and 2-AB are not included as part of the GlycoWorks Reagent Kit.

## EXPERIMENTAL

### Sample Description

For the labeled oligosaccharide recovery studies, the Glycan Performance Test Standard ([p/n 186006349](#)) was mixed with 2-AB labeled trisialylated A3 (ProZyme) in water to make a solution of 3 pmol/μL. Aliquots (10 μL) of this mixture were diluted with 15 μL of acetonitrile (ACN) to make control samples. Aliquots (10 μL) were also dried under vacuum to prepare lyophilization control samples. In addition, 10-μL aliquots were processed by HILIC SPE according to the protocol found in the GlycoWorks High-throughput Sample Preparation Kit Care and Use Manual ([p/n 715004079](#)). Various eluents were studied and are noted in Figures 3 through 6. Dried glycans were reconstituted in 10 μL of water and 15 μL of ACN prior to injection.

For the unlabeled oligosaccharide recovery studies, unlabeled Man5 and trisialylated A3, obtained from ProZyme, were reconstituted in water, and mixed to equal molarity (6.7 μM). Aliquots (6 μL) of this mixture were diluted with 6 μL of ACN to make control samples. Aliquots (6 μL) were also dried under vacuum to prepare lyophilization controls. In addition, 6 μL aliquots were processed by HILIC SPE, according to the protocol found in the GlycoWorks High-throughput Sample Preparation Kit Care and Use Manual. Elution was performed with an eluent comprised of 100 mM ammonium acetate (NH<sub>4</sub>OAc) in 5% ACN (pH 7). Dried glycans were reconstituted in 6 μL of water and 6 μL of ACN prior to injection.

A schematic for the HILIC SPE steps used in this study is shown below:

<b>WASH</b> 200 μL H <sub>2</sub> O
<b>CONDITION</b> 200 μL 85% ACN
<b>LOAD</b> 10 μL sample + 100 μL ACN (2-AB labeled) 6 μL sample + 44 μL 25 mM NH <sub>4</sub> HCO <sub>3</sub> (pH 8) + 350 μL ACN (unlabeled)
<b>WASH</b> 3 x [200 μL 85% ACN]
<b>ELUTE</b> 3 x [50 μL 100 mM NH <sub>4</sub> OAc, 5% ACN, pH 7] (unless otherwise noted)
<b>LYOPHILIZE AND RECONSTITUTE</b>

*Note: Eluates were transferred to micro-centrifuge tubes then lyophilized. Thereafter, samples were reconstituted and transferred to sample vials for injection.*

The procedure for preparing samples for this analysis can be complicated. GlycoWorks products help make the workflow more straightforward by bringing together many of the needed consumables. Moreover, GlycoWorks products provide a solution to the cleanup steps that are needed throughout the process of preparing labeled glycans for analysis. In particular, HILIC solid-phase extraction (SPE)<sup>11,12</sup> has been developed to purify released glycans from proteins and buffer/formulation constituents, which can disrupt derivatization. HILIC SPE can also purify labeled glycans after derivatization from excess reagents, which can potentially interfere with downstream chromatography, reduce the lifetime of a column, and thereby impair method robustness.

This application note evaluates HILIC SPE sample preparation to ensure quantitative recovery of both unlabeled and labeled N-glycans. A test mixture, including a complex array of 2-AB labeled human IgG glycans spiked with both high mannose and trisialylated glycans, was used to interrogate and optimize SPE recoveries as well as study the robustness of optimized elution conditions. In addition, an LC/MS assay was employed to demonstrate the quantitative recovery of unlabeled glycans during HILIC SPE with the optimized conditions.

**Method conditions** (unless otherwise noted)**LC conditions**

System:	ACQUITY UPLC H-Class Bio with a 20-cm Column Heater
Detection:	Waters® ACQUITY UPLC FLR Detector
Excitation:	330 nm
Emission:	420 nm
Scan rate:	10 Hz
Time constant:	0.2 s
Gain:	1.00
Column:	ACQUITY UPLC GST Amide (BEH Glycan), 1.7 µm, 2.1 x 150 mm ( <a href="#">p/n 186004742</a> )
Column temp.:	60 °C
Sample temp.:	15 °C
Injection volume:	2.5 µL (HILIC-FLR), 10 µL (HILIC-MS)
Flow rate:	0.5 mL/min (0.25 mL/min for the highly aqueous regeneration step in the gradient)
Mobile phase A:	100 mM Ammonium formate, pH 4.4
Mobile phase B:	Acetonitrile (ACN)
Sample collection plate:	1 mL Round Well Collection Plate ( <a href="#">p/n 186002481</a> )
Vials:	LCGC Certified Clear Glass 12 x 32 mm Screw Neck Qsert Vial ( <a href="#">p/n 186001126C</a> )

## Gradients:

HILIC-FLR	Time (min)	% A	% B	Flow rate (mL/min)
	0	22.0	78.0	0.5
	38.5	44.1	55.9	0.5
	39.5	80.0	20.0	0.25
	44.5	80.0	20.0	0.25
	46.5	22.0	78.0	0.5
	50.0	22.0	78.0	0.5
HILIC-MS	Time (min)	% A	% B	Flow rate (mL/min)
	0	27.9	72.1	0.5
	19.25	50.0	50.0	0.5
	20.25	80.0	20.0	0.25
	25.25	80.0	20.0	0.25
	27.25	22.0	78.0	0.5
	31.00	22.0	78.0	0.5

**MS conditions**

Mass spectrometer:	Xevo® G2 QTof
Ionization mode:	ESI+
Analyzer mode:	Sensitivity
Capillary voltage:	3.20 kV
Cone voltage:	37 V
Source temp.:	100 °C
Desolvation temp.:	350 °C
Cone gas flow:	0.0 L/h
Desolvation gas flow:	800 L/h
Calibration:	NaI, 1 µg/µL from 50 to 2000 <i>m/z</i>
Acquisition:	700 to 3000 <i>m/z</i> , 1 Hz scan rate
Lock mass:	0.5 µM [Glu <sup>1</sup> ]-fibrinopeptide in 50:50 ACN/water, 0.1% formic acid

**Data management**

UNIFI® and MassLynx® software

## RESULTS AND DISCUSSION

## Optimizing the recovery of glycans from GlycoWorks HILIC SPE

A test mixture, capable of rigorously interrogating the recovery of N-glycans from GlycoWorks HILIC SPE, was prepared by combining the Glycan Performance Test Standard with 2-AB labeled trisialylated A3 glycans. The Glycan Performance Test Standard is comprised of 2-AB labeled N-glycans derived from pooled human serum IgG spiked with high mannose glycans (Man5 and Man6). The addition of the trisialylated A3 glycans further extends the complexity of this mixture, as the A3 glycans are larger, more acidic, and bind more strongly in a HILIC-based separation than glycans commonly found on human or human-like IgG. Figure 2 shows a HILIC-FLR analysis of this modified test mixture using an ACQUITY UPLC GST Amide (BEH Glycan) Column along with UNIFI Software for instrument control and data interpretation.

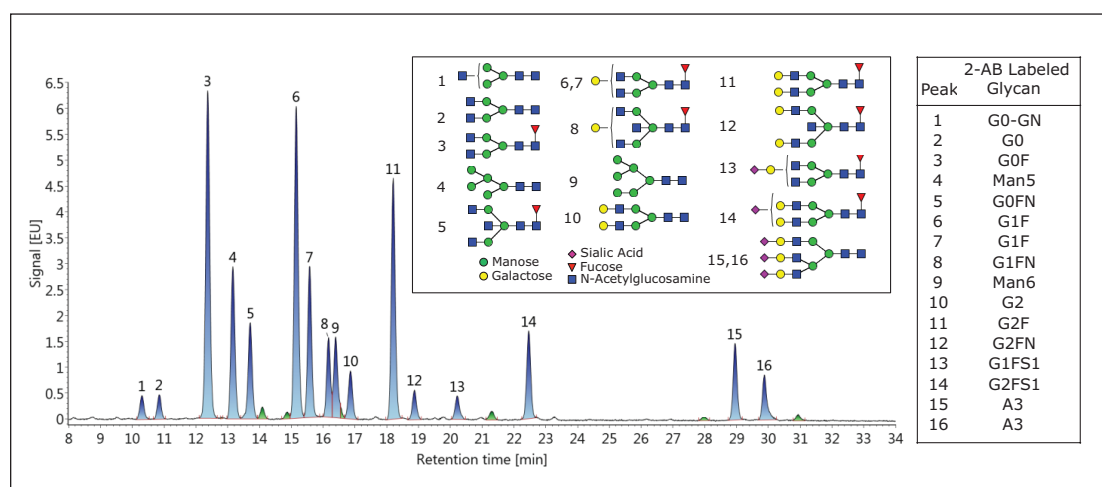


Figure 2. HILIC-FLR analysis of 2-AB labeled glycan performance test standard and trisialylated A3 glycans. 3 pmol of sample injected in 2.5  $\mu$ L onto an ACQUITY UPLC GST Amide (BEH Glycan), 1.7  $\mu$ m, 2.1 x 150 mm Column. Peaks detected by UNIFI processing are shaded in blue (expected component) or green (discovered component).



Based on this analytical approach, the HILIC SPE of the GlycoWorks solution was evaluated. A silica-based aminopropyl sorbent is contained in the GlycoWorks Kit ([p/n 176003090](#)). This sorbent was selected from several tested because it is highly polar and, consequently, useful for HILIC separations. Since this sorbent possesses a weakly basic surface and potential for anion exchange, it was, however, assumed that the relative and total recovery of glycans from a GlycoWorks HILIC SPE device could be particularly sensitive to elution conditions. To evaluate this step, elution from the GlycoWorks HILIC sorbent was studied in detail. 2-AB labeled glycans were loaded onto a 96-well HILIC  $\mu$ Elution Plate according to the protocol provided in the GlycoWorks High-throughput Sample Preparation Kit Care and Use Manual.<sup>13</sup> Various eluents were then employed for elution of the labeled glycans, and recoveries for each major species in the test mixture was subsequently determined. These data were compared alongside the recoveries of the glycans from just the lyophilization and reconstitution steps that were performed after the HILIC SPE procedure, in preparation of the samples for HILIC-FLR. A series of eluents comprised of 20% ACN and increasing concentrations of ammonium bicarbonate ( $\text{NH}_4\text{HCO}_3$ , pH 8–9) were first investigated. A volatile salt was chosen, due to requisite lyophilization steps. Interpretation of the recoveries led to the observation that the recovery of the glycans was biased, based on eluent choice, with smaller, neutral species recovered better than larger, acidic species. With an eluent comprised of simply 20% ACN/80% water ( $\text{H}_2\text{O}$ ) and no other components, acidic glycans in the test mixture were either poorly recovered or not recovered at all; meanwhile, neutral glycans were obtained with reasonable recovery ( $\geq 70\%$ ). The addition of  $\text{NH}_4\text{HCO}_3$ , to concentrations of 25 mM or higher minimized this apparent and non-desired ionic retention mechanism. Nevertheless, even with 100 mM  $\text{NH}_4\text{HCO}_3$ , there was a noticeable correlation between recovery and the hydrophilicity, or glucose unit (GU) values, of the glycans (Figure 3A).

Biased recovery, or speciation, can be problematic for a sample preparation procedure. In addition to not providing an accurate representation of the species present in the sample, it can be indicative of a method that is not robust and that the relative abundance profiles obtained may not be reproducibly determined, particularly with respect to the most poorly recovered species. As a result, a study was performed to improve these observed 2-AB labeled glycan recoveries. Given that retention of polar analytes to a polar sorbent is dominated by hydrogen bonding and ionic interactions, eluents with more aqueous content (decreased ACN concentrations) were evaluated (Figure 3B). As predicted,  $\text{NH}_4\text{HCO}_3$  eluents comprised of lower concentrations of organic solvent yielded both higher and less biased recoveries of the glycan profile. Within the range of this study, an eluent composition of 25 mM  $\text{NH}_4\text{HCO}_3$ /5% ACN was found to produce optimal recoveries.

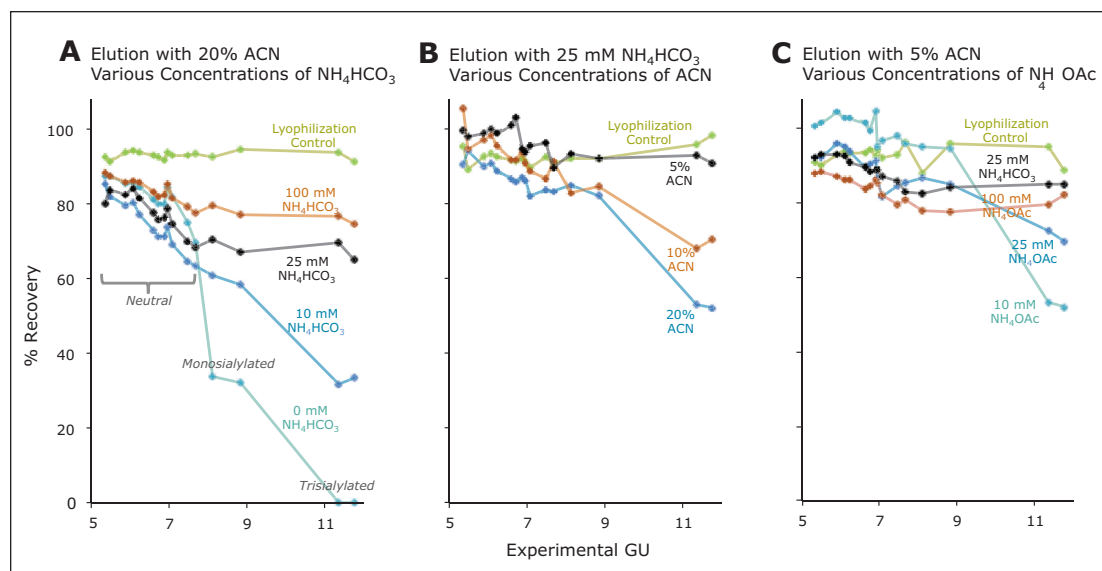


Figure 3. Recovery of 2-AB labeled N-glycans (Figure 2) from GlycoWorks HILIC SPE 96-well  $\mu$ Elution Plates (30 pmol of glycans processed). Percent recoveries as a function of experimentally determined glucose units (GU) are shown for various elution conditions. Values are based on the average of three replicate analyses.

Unfortunately, eluents containing  $\text{NH}_4\text{HCO}_3$  posed a challenge in this application as their basicity (typically pH 8 but increased toward pH 9 upon exposure to air) may result in noticeable dissolution of the silica SPE particles and problematic levels of precipitate in the reconstituted samples. To eliminate this potential issue and establish a more robust procedure, we investigated alternative eluents based on neutral solutions of ammonium acetate (pH 7). The effect of ammonium acetate ( $\text{NH}_4\text{OAc}$ ) eluents on the recoveries of the 2-AB labeled glycans is shown in Figure 3. A 100-mM  $\text{NH}_4\text{OAc}$ , 5% ACN eluent was selected as the optimal elution condition, since it provided high as well as relatively unbiased analyte recoveries, similar to those obtained using the 25-mM  $\text{NH}_4\text{HCO}_3$ , 5% ACN eluent.

The set of chromatograms shown in Figures 4A and 4B demonstrates that the test mixture, before and after HILIC SPE treatment, exhibits highly consistent glycan profiles. Relative abundance determinations for control samples as well as a processed sample are shown in Figure 4C. Compared to the control, differences in relative abundances were  $\leq 7\%$  across the entire profile. For example, the relative abundance of GOF (peak 3) was determined to be 17.9% and 18.6%, before and after SPE, respectively. The relative abundance of trisialylated A3 (peak 16) before and after SPE was 2.8% and 2.7%, respectively (Figure 4C). These optimized elution conditions provide quantitative recoveries for both glycans typical of human IgGs and heavily sialylated glycans, as demonstrated with the recovery of the A3 glycan. With these conditions, the GlycoWorks HILIC  $\mu$ Elution Plate is well suited for the preparation of N-glycans from a range of glycoproteins, including those with primarily low GU value neutral glycans as well as those decorated with high GU value, heavily sialylated glycans.

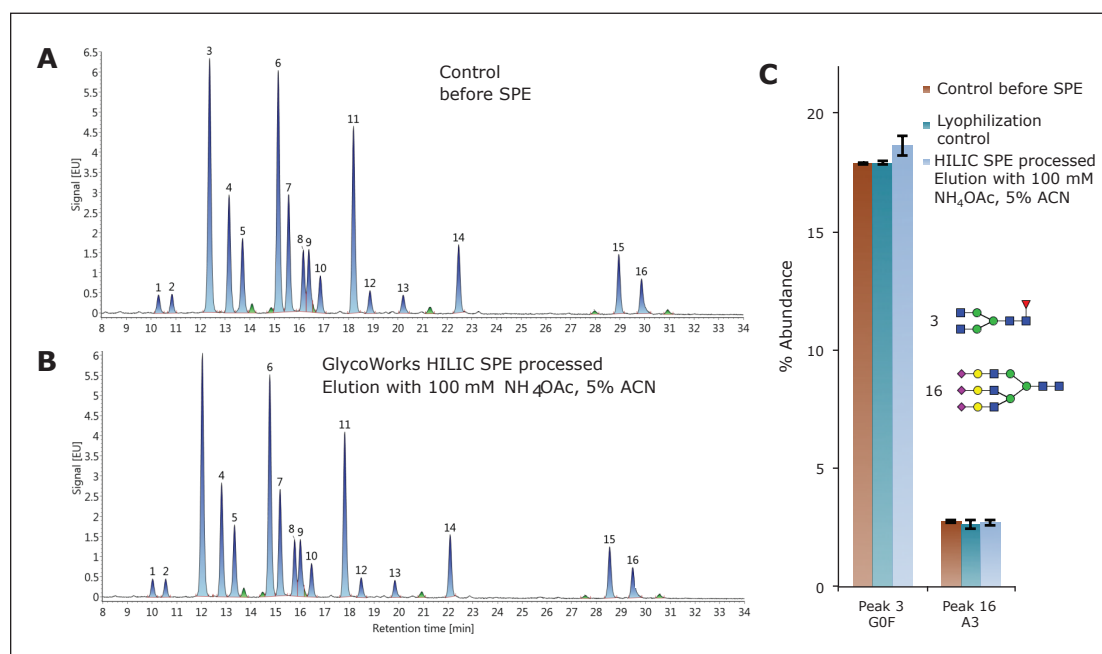


Figure 4. Glycan profile (A) before, and (B) after GlycoWorks HILIC SPE with the optimized elution conditions. Representative chromatograms and relative abundances (C) measured for two 2-AB labeled glycans (low and high GU values) from the test mixture before and after GlycoWorks HILIC SPE are displayed ( $n=3$ ).

### Robustness testing of optimized SPE elution conditions

The GlycoWorks HILIC  $\mu$ Elution Plate was optimized to yield desired recoveries and, more importantly, to be robust. Elution conditions were purposely optimized so that even relatively large changes in critical elution parameters, namely organic concentration and ionic strength, would have minimal effect on the obtained glycan profile. To demonstrate this, the HILIC SPE method was subjected to robustness testing. Glycan profiles obtained using SPE eluents with the optimized concentrations of ACN and  $\text{NH}_4\text{OAc}$  concentrations were compared to those obtained with eluents comprised of ACN and  $\text{NH}_4\text{OAc}$  concentrations varied by 10%. The impact of changes in ionic strength and ACN concentration were purposely compounded in these studies. A strong eluent with 110-mM  $\text{NH}_4\text{OAc}$ , 4.5% ACN as well as a comparatively weak eluent with 90-mM  $\text{NH}_4\text{OAc}$ , 5.5% ACN were employed. Figure 5 shows the relative abundances for each of the major constituents in the test mixture obtained using these varied conditions. The glycan profiles obtained were comparable to the conditions tested. The largest percent change observed between relative abundances from the optimal to extreme conditions was only 7%, corresponding to the recovery of trisialylated A3 (peak 16). This result demonstrates that clean-up of 2-AB labeled glycans using the GlycoWorks HILIC  $\mu$ Elution Plate with the optimized elution conditions exhibits noteworthy ruggedness, and is, therefore a robust solution for N-glycan preparations even in quality control applications.

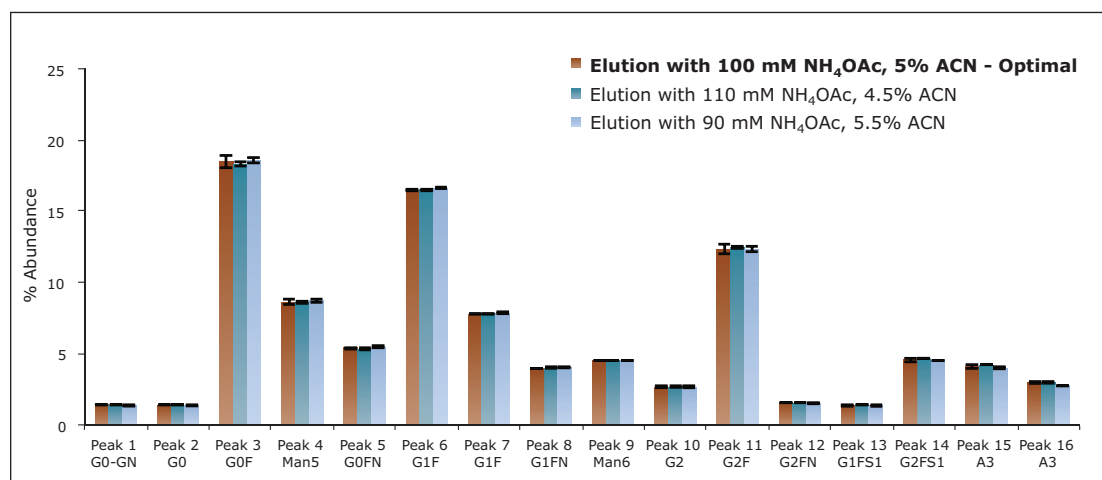


Figure 5. Robustness testing of the SPE elution conditions. Glycan profile for the test mixture obtained after GlycoWorks HILIC SPE with the optimized elution conditions and elution conditions wherein critical parameters were varied by 10% ( $n=3$ ).

## Assaying unlabeled glycans before and after GlycoWorks HILIC SPE by LC/MS

The GlycoWorks HILIC  $\mu$ Elution Plate is also suggested for the initial purification of unlabeled glycans cleaved from the target glycoprotein via enzymatic digestion. 2-AB labeled glycans, as previously studied, are slightly less hydrophilic than unlabeled glycans due to the hydrophobicity of the benzamide fluorescent tag. To confirm that recoveries of unlabeled glycans were similar in comparison to the recoveries of 2-AB labeled glycans, an additional study was performed. A HILIC-MS assay was established to determine the relative abundances of two unlabeled glycans representing the extremes of most IgG N-glycan profiles. The mixture tested was comprised of equal amounts of a neutral, low GU value glycan (Man5) and an acidic, high GU value glycan (trisialylated A3). An extracted ion chromatogram (XIC) obtained for this mixture with a Xevo G2 QTof is shown in Figure 6A. Interestingly, two major peaks were observed for both unlabeled Man5 and A3, indicating the presence of different isoforms. Mass spectral windows wide enough to capture both protonated and salt adduct species of the unlabeled glycans were used to construct the chromatogram. XICs obtained in this manner were integrated, and the obtained peak areas were used to calculate relative abundances of the unlabeled glycans before and after HILIC SPE (Figure 6B). As with 2-AB labeled glycans, the profile of the unlabeled glycan mixture before and after SPE was highly comparable, indicating that the optimized GlycoWorks HILIC SPE process also yields minimally biased recoveries of unlabeled glycans.

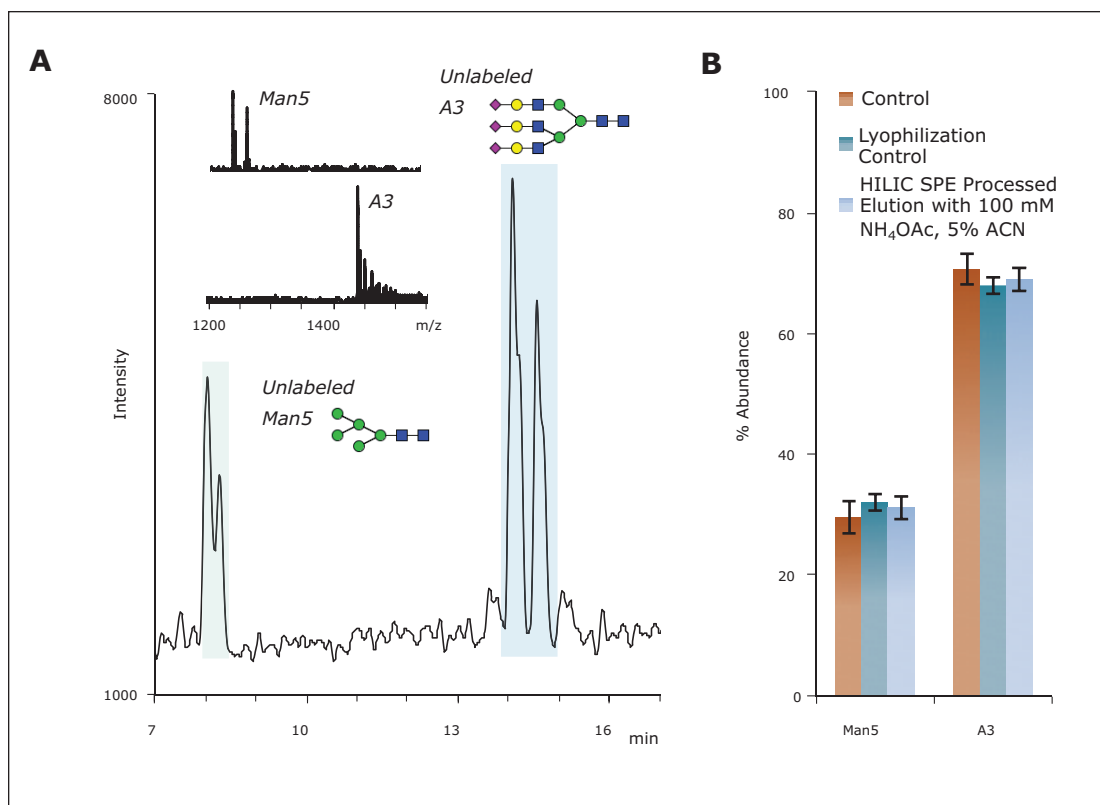


Figure 6. Assessing the effect of GlycoWorks HILIC SPE on the distribution of unlabeled glycans. An extracted ion chromatogram (XIC, 1235-1270+1435-1500  $m/z$ ) from a HILIC-ESI-MS analysis of a mixture containing a low GU, neutral glycan (Man5) and a high GU, acidic glycan (trisialylated A3) is shown on the left (A). Relative abundances determined via such an analysis for the mixture before and after GlycoWorks HILIC SPE are shown on the right (B). In this study, 40 pmol of each unlabeled glycan were processed by GlycoWorks HILIC SPE and 10  $\mu$ L of a 12- $\mu$ L reconstitution for a total maximum load of 33 pmol of each glycan was loaded onto an ACQUITY UPLC GST Amide (BEH Glycan), 1.7  $\mu$ m, 2.1  $\times$  150 mm Column for analysis.



## CONCLUSIONS

HILIC SPE was rigorously studied and optimized to provide quantitative recoveries of 2-AB labeled and unlabeled N-glycans. A test mixture containing a diverse array of 2-AB labeled N-glycans was employed to interrogate GlycoWorks HILIC  $\mu$ Elution Plate performance, and develop optimized elution conditions for a robust and reproducible method. In ruggedness testing of the optimized SPE, only minimal changes in a glycan profile were observed despite significant changes in the critical parameters of the SPE eluent. Moreover, an LC/MS assay showed that unlabeled glycans, like 2-AB labeled glycans, are recovered with minimal bias using the newly optimized elution conditions. These studies highlight the development of the GlycoWorks solution and its value in facilitating the release, labeling, and purification of N-glycans.

## References

1. Apweiler R, Hermjakob H, Sharon N. On the frequency of protein glycosylation, as deduced from analysis of the SWISS-PROT database. *Biochim Biophys Acta*. 1999; 1473(1): 4-8.
2. Hart GW. Glycosylation. *Curr Opin Cell Biol*. 1992; 4(6): 1017-23.
3. Marino K, Bones J, Kattla JJ, Rudd PM. A systematic approach to protein glycosylation analysis: a path through the maze. *Nat Chem Biol*. 2010; 6(10): 713-23.
4. Kaneshiro K, Watanabe M, Terasawa K, Uchimura H, Fukuyama Y, Iwamoto S, Sato TA, Shimizu K, Tsujimoto G, Tanaka K. Rapid quantitative profiling of N-glycan by the glycan-labeling method using 3-aminoquinoline/ $\alpha$ -cyano-4-hydroxycinnamic acid. *Anal Chem*. 2012; 84(16): 7146-51.
5. Ahn J, Bones J, Yu YQ, Rudd PM, Gilar M. Separation of 2-aminobenzamide labeled glycans using hydrophilic interaction chromatography columns packed with 1.7 microm sorbent. *J Chromatogr B Analyt Technol Biomed Life Sci*. 2010; 878(3-4): 403-8.
6. Yu YQ, Ahn J, Gilar M. Trastuzumab Glycan Batch-to-Batch Profiling using a UPLC/FLR/MS Mass Spectrometry Platform. Waters Application Note [720003576en](#). 2010 June.
7. Hilliard M, Struwe W, Carta G, O'Rourke J, McLoughlin N, Rudd P, Yu YQ. A Systematic Approach to Glycan Analysis Using HILIC-UPLC and an Online Database of Standardized Values. Waters Application Note [720004203en](#). 2012 December.
8. Hilliard M, Struwe W, Adamczyk B, Saldova R, Yu YQ, O'Rourke J, Carta G, Rudd P. Development of a Glycan Database for Waters ACQUITY UPLC Systems. Waters Application Note [720004202en](#). 2012 Sept.
9. Yu YQ. Analysis of N-Linked Glycans from Coagulation Factor IX, Recombinant and Plasma Derived, Using HILIC UPLC/FLR/QToF MS. Waters Application Note [720004019en](#). 2011 June.
10. Gillece-Castro B, Tran KV, Turner JE, Wheat TE, Diehl DM. N-Linked Glycans of Glycoproteins: A New Column for Improved Resolution. Waters Application Note [720003112en](#). 2009 June.
11. Yu YQ, Gilar M, Kaska J, Gebler JC. A rapid sample preparation method for mass spectrometric characterization of N-linked glycans. *Rapid Commun Mass Spectrom*. 2005; 19(16): 2331-6.
12. Yu YQ, Gilar M, Kaska J, Gebler JC. A Deglycosylation and Sample Cleanup Method for Mass Spectrometry Analysis of N-linked Glycans. Waters Application Note [720001146en](#). 2007 May.
13. GlycoWorks High-Throughput Sample Preparation Kit. *Waters Care and Use Manual* [715004079](#). 2013.

# Waters

THE SCIENCE OF WHAT'S POSSIBLE.™

Waters, ACQUITY UPLC, Xevo, UNIFI, and MassLynx are registered trademarks of Waters Corporation. GlycoWorks and The Science of What's Possible are trademarks of Waters Corporation. All other trademarks are the property of their respective owners.

©2013 Waters Corporation. Produced in the U.S.A.  
June 2013 720004717EN LL-PDF

**Waters Corporation**  
34 Maple Street  
Milford, MA 01757 U.S.A.  
T: 1 508 478 2000  
F: 1 508 872 1990  
[www.waters.com](http://www.waters.com)

