


RapiFluor-MS Facilitates Versatile Detection of Released N-Glycans

Matthew A. Lauber, Stephan M. Koza, and Erin E. Chambers

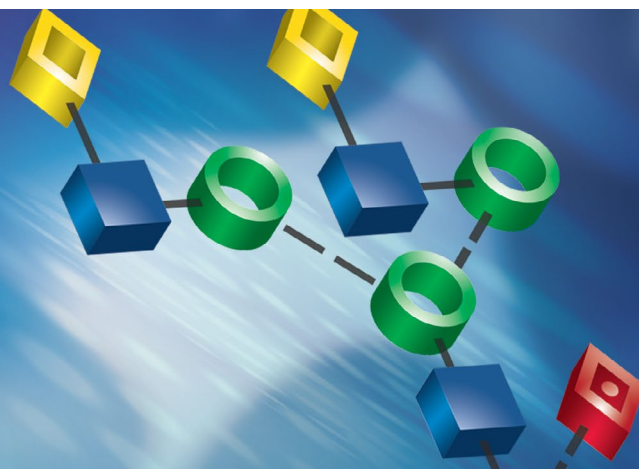

GOAL

To demonstrate that *RapiFluor-MS*TM labeled N-glycans can be readily detected by fluorescence, mass spectrometry as well as UV absorbance.

BACKGROUND

Elucidating information about protein N-glycosylation can give insights into disease¹⁻³ and the structure-function properties of biopharmaceuticals.⁴⁻⁵ In previous approaches to N-glycan analysis, analysts relied on laborious preparation techniques, which established a barrier between samples of interest and analytical results.⁶⁻⁷ The recent development of the GlycoWorksTM *RapiFluor-MS* N-Glycan Kit has alleviated numerous shortcomings of conventional sample preparations by streamlining and accelerating both the enzymatic release and labeling of N-glycans. In addition, the properties of the novel *RapiFluor-MS* labeling reagent now make it possible to obtain released glycan profiles by hydrophilic interaction chromatography (HILIC) with inordinately high sensitivity. The *RapiFluor-MS* labeling reagent was designed with an efficient quinoline fluorophore and a highly basic tertiary amine to enable fluorescence and mass spectrometric (MS) detection (Figure 1). By virtue of being an extensively conjugated fluorophore, the *RapiFluor-MS* label is also highly chromogenic such that it exhibits reasonably high UV absorptivity. In this work, it is demonstrated that this attribute of the *RapiFluor-MS* label facilitates the detection of released N-glycans by not only fluorescence and MS detection but also UV absorbance.

The unique properties of the *RapiFluor-MS* label can be exploited to detect N-glycans by fluorescence, mass spectrometry, and UV absorbance.

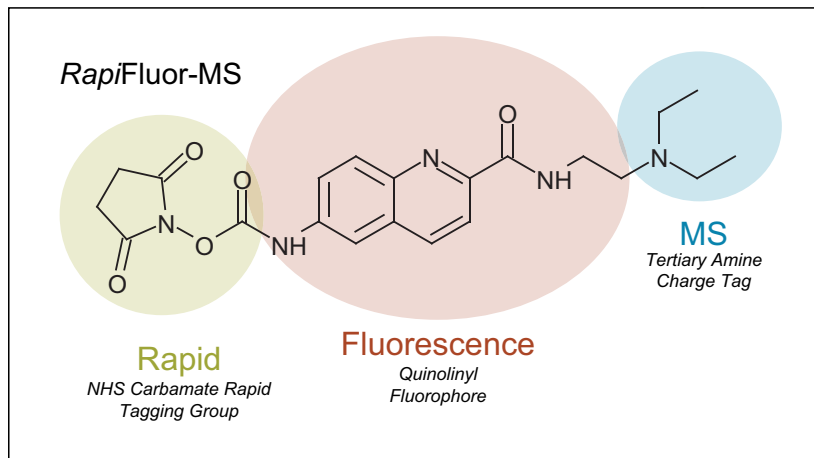


Figure 1. Chemical structure of *RapiFluor-MS*.

THE SOLUTION

RapiFluor-MS labeled glycans prepared from pooled human IgG were analyzed by HILIC and three different modes of detection: UV, fluorescence, and MS. To approximate method sensitivity, these N-glycans were separated at total mass loads ranging from 0.02 to 20 pmols, and to have direct correspondence between data sets, detection was performed serially from UV to fluorescence to MS.

Figure 2 displays the chromatograms from each detection mode. Results from increasingly higher mass loads are shown across the figure from left to right. As can be seen through observation of the middle chromatograms, as little as 20 fmols of a *RapiFluor*-MS N-glycan pool can be readily visualized by fluorescence detection. This corresponds to a limit of detection (LOD) that is remarkably low for an individual *RapiFluor*-MS N-glycan species, a value corresponding to ≤ 1 fmol. As evidenced by the top chromatograms, MS sensitivity is likewise noteworthy. Using a Xevo® G2-XS QToF mass spectrometer, *RapiFluor*-MS N-glycans were detected on base peak intensity (BPI) chromatograms down to individual glycan quantities of approximately 10 fmols. That informative mass information can be produced at such low levels alongside the limits of fluorescence detection is a testament to the design of the *RapiFluor*-MS label.

Yet, what is of interest here is UV-based detection, for which representative data are shown with the bottom chromatograms. These data clearly demonstrate that *RapiFluor*-MS labeled glycans can be detected via their UV absorbance, albeit with reduced sensitivity. N-glycans were detectable by UV at a 2 pmol load of an IgG glycan pool with a limit of detection for single species of about 100 fmols. Interestingly, this could be sufficient sensitivity for some applications of released glycan analysis. The GlycoWorks *RapiFluor*-MS N-Glycan Kit allows for the analysis of 5 pmols up to about 20 pmols of IgG glycans without the need for evaporation and concentration, which helps to make it practical to implement UV detection.

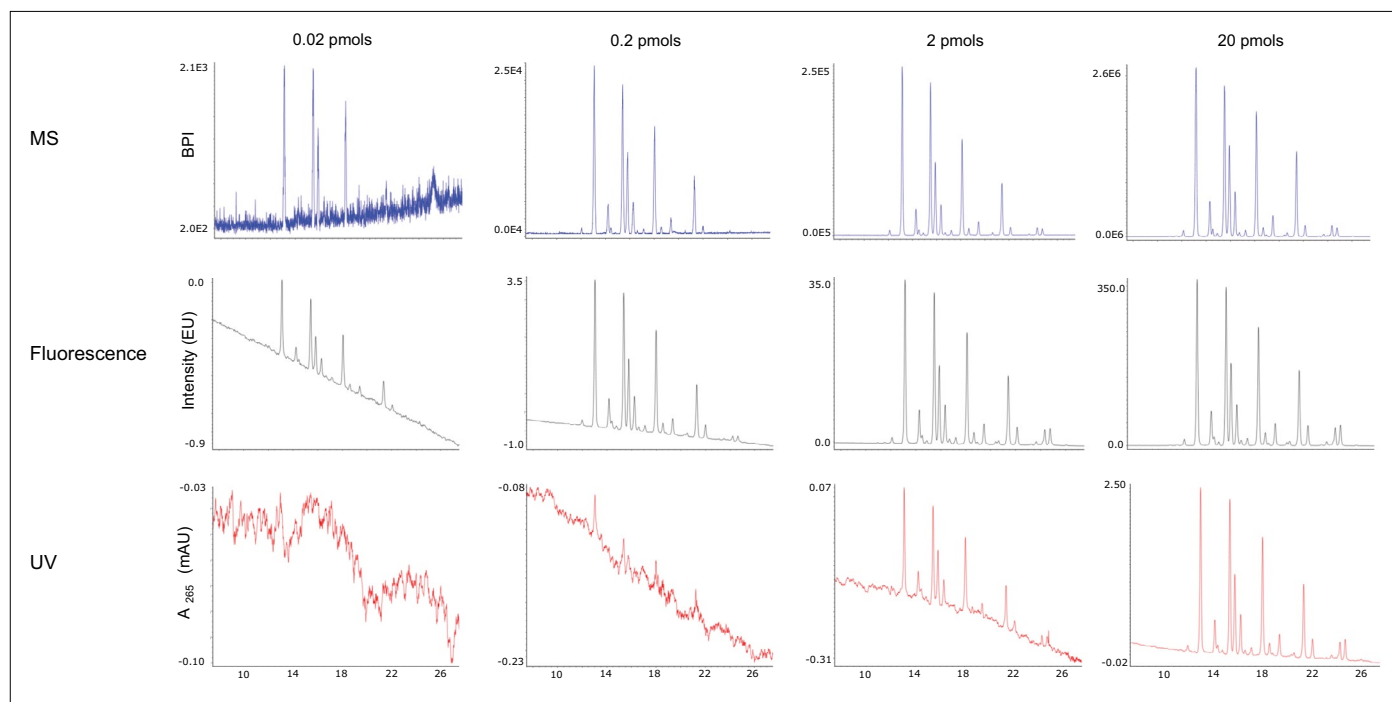


Figure 2. *RapiFluor*-MS N-glycans at varying mass loads as profiled by HILIC using MS, fluorescence, and UV detection. Analyses were performed with an ACQUITY UPLC® H-Class Bio System and a Xevo G2-XS QToF using the *RapiFluor*-MS N-Glycan Kit (p/n [176003606](#)), the ACQUITY UPLC Glycan BEH Amide Column, 130Å, 1.7 µm, 2.1 x 150 mm (p/n [186004742](#)) and the method described in the *RapiFluor*-MS N-Glycan Kit Care and Use Manual ([715004793EN](#)). Samples were injected at varying quantities, corresponding to the N-glycans derived from 0.02, 0.2, 2, and 20 pmols of pooled human IgG (*RapiFluor*-MS Glycan Performance Test Standard (p/n [186007983](#))).

Here, a 20 pmol load of IgG glycans was indeed able to produce an adequately sensitive UV profile for relative quantitation. Figure 3A shows a comparison of the 20 pmol IgG N-glycan profile as obtained by UV versus fluorescence detection. Undoubtedly, fluorescence yields a higher quality profile that could more easily support investigations into very low abundance glycans, such as those below 0.1% relative abundance. Nevertheless, as shown in Figure 3B, the UV profile proved to give comparable determinations for species above 0.2% relative abundance.

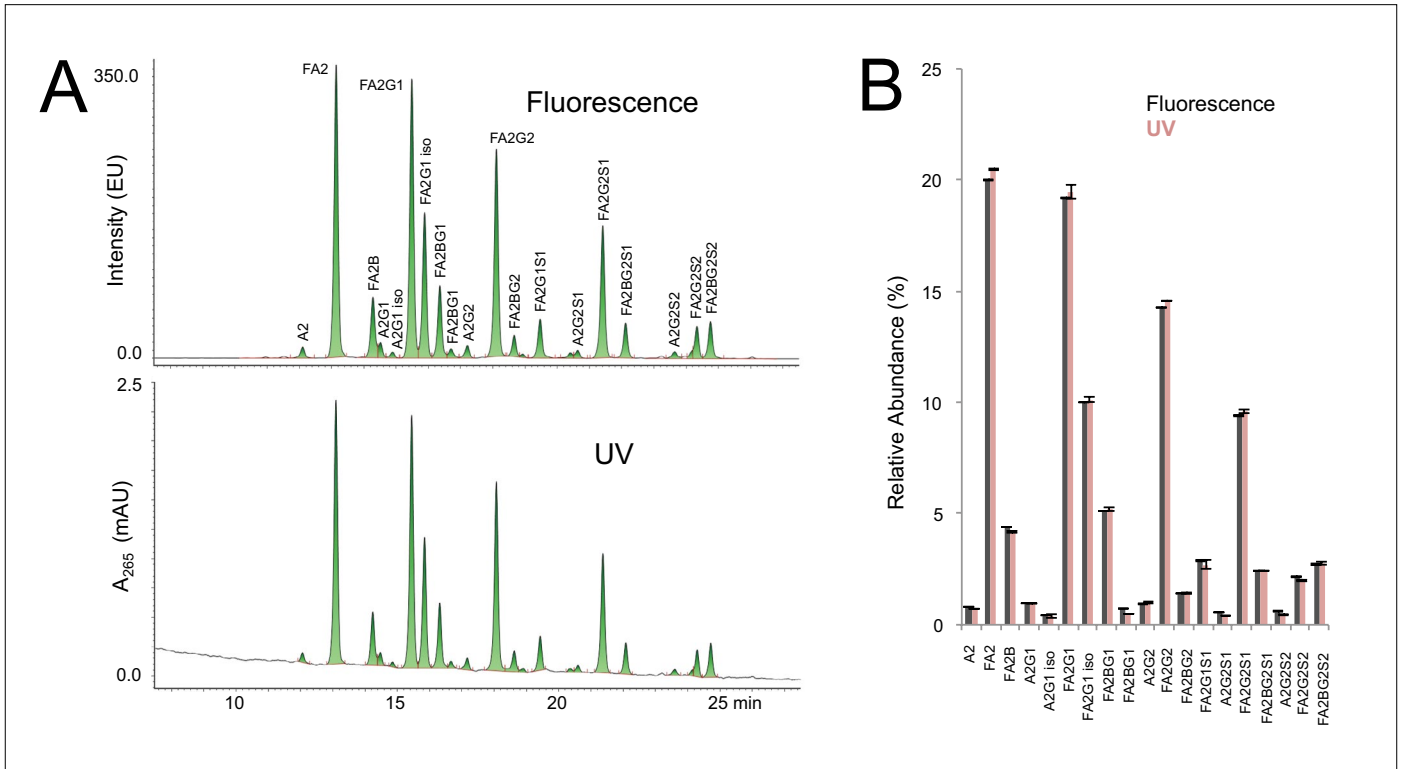


Figure 3. Relative quantitation as performed with UV versus fluorescence detection. (A) UV and fluorescence chromatograms obtained for 20 pmols of RapiFluor-MS Glycan Performance Test Standard (p/n [186007983](#)). (B) Relative abundances of the 19 most abundant glycan species.

SUMMARY

The unique properties of the *RapiFluor*-MS label can be exploited to detect N-glycans by both fluorescence and mass spectrometry, and, as we now show, by UV absorbance. Fluorescence, with its LOD of ≤ 1 fmol, offers the most robust sensitivity for chromatographic detection. Modern QToF mass spectrometry is sensitive down to quantities of about 10 fmols using analytical scale chromatography. UV detection, meanwhile, produces interpretable signal for a 100 fmol quantity of an individual *RapiFluor*-MS glycan. While there is an order of magnitude difference among their limits of detection, each detection mode could potentially be implemented to interrogate an N-glycan sample. One advantage that UV absorbance has over fluorescence and MS is that the measured peak heights and areas are comparable between LC systems for a defined separation when corrected for flow cell path length. Such versatile detection can be taken advantage of to troubleshoot instrumentation or to implement released glycan analysis where there may be limited options available for instrumentation.

References

1. Ohtsubo, K.; Marth, J. D., Glycosylation in cellular mechanisms of health and disease. *Cell* **2006**, 126 (5), 855–67.
 2. Mechref, Y.; Hu, Y.; Garcia, A.; Zhou, S.; Desantos-Garcia, J. L.; Hussein, A., Defining putative glycan cancer biomarkers by MS. *Bioanalysis* **2012**, 4 (20), 2457–69.
 3. Ruhaak, L. R.; Miyamoto, S.; Lebrilla, C. B., Developments in the identification of glycan biomarkers for the detection of cancer. *Mol Cell Proteomics* **2013**, 12 (4), 846–55.
 4. Dalziel, M.; Crispin, M.; Scanlan, C. N.; Zitzmann, N.; Dwek, R. A., Emerging principles for the therapeutic exploitation of glycosylation. *Science* **2014**, 343 (6166), 1235681.
 5. Beck, A.; Wagner-Rousset, E.; Ayoub, D.; Van Dorsselaer, A.; Sanglier-Cianferani, S., Characterization of therapeutic antibodies and related products. *Anal Chem* **2013**, 85 (2), 715–36.
 6. Mechref, Y.; Hu, Y.; Desantos-Garcia, J. L.; Hussein, A.; Tang, H., Quantitative glycomics strategies. *Mol Cell Proteomics* **2013**, 12 (4), 874–84.
- Ruhaak, L. R.; Zauner, G.; Huhn, C.; Bruggink, C.; Deelder, A. M.; Wuhrer, M., Glycan labeling strategies and their use in identification and quantification. *Anal Bioanal Chem* **2010**, 397 (8), 3457–81.

Waters

THE SCIENCE OF WHAT'S POSSIBLE.®

Waters, The Science of What's Possible, ACQUITY UPLC, and Xevo are registered trademarks of Waters Corporation. GlycoWorks and *RapiFluor*-MS are trademarks of Waters Corporation. All other trademarks are the property of their respective owners.

©2016 Waters Corporation. Produced in the U.S.A. March 2016 720005646EN AW-PDF

Waters Corporation
34 Maple Street
Milford, MA 01757 U.S.A.
T: 1 508 478 2000
F: 1 508 872 1990
www.waters.com