

Fast Determination of Inorganic Counterions in a Pharmaceutical Drug Using High-Pressure Capillary Ion Chromatography

Fei Pang, Terri Christison and Linda Lopez, Thermo Fisher Scientific Inc., Sunnyvale, CA, USA

Introduction

One of the most important applications of ion chromatography (IC) is the determination of counterions in active pharmaceutical ingredients (APIs) and in drug products in pharmaceutical industry.¹ Approximately 50% of drugs on the market are developed in salt forms.^{2,3} Certain physicochemical and biopharmaceutical properties of APIs can be improved by pairing a basic or acidic drug molecule with a counterion to create a salt version of the drug with high solubility, stable crystalline form, and good bioavailability. Ion chromatography with suppressed conductivity detection plays an important role in the salt selection process to establish correct molecular mass of the entity in early stages of drug development. IC can also be used in quality control to verify identity, strength, and purity of ionic APIs.

This application brief describes the determination of counter anion chloride in a drug for type 2 diabetes treatment with the Thermo Scientific Dionex ICS-5000 Capillary HPIC system, which can operate at backpressures up to 5000 psi. This capability facilitates higher sample throughput by simply increasing the flow rate. As shown in Figure 1, the analysis of a counterion can be achieved in less than 8 min at 24 $\mu\text{L}/\text{min}$ compared to 15 min at a 12 $\mu\text{L}/\text{min}$ flow rate using a Thermo Scientific Dionex IonSwift MAX-100 capillary column and suppressed conductivity detection. The Dionex IonSwift™ MAX-100 column uses monolith technology and is designed for the separation of small molecules and inorganic anions using a hydroxide gradient delivered by an eluent generator. At a 24 $\mu\text{L}/\text{min}$ flow rate, about 4500 psi backpressure is generated.

Scaling down from standard bore to capillary scale brings many benefits to IC users. One of the most important values is that the system can be left always on and ready for analysis because of its low consumption of eluent (15 mL of source water a day at 10 $\mu\text{L}/\text{min}$ flow rate). The amount of waste generated is significantly decreased and the Thermo Scientific Dionex Eluent Generation Cartridge producing the eluent lasts 18 months under typical conditions in continuous operation mode, which translates into reduced overall cost of ownership.

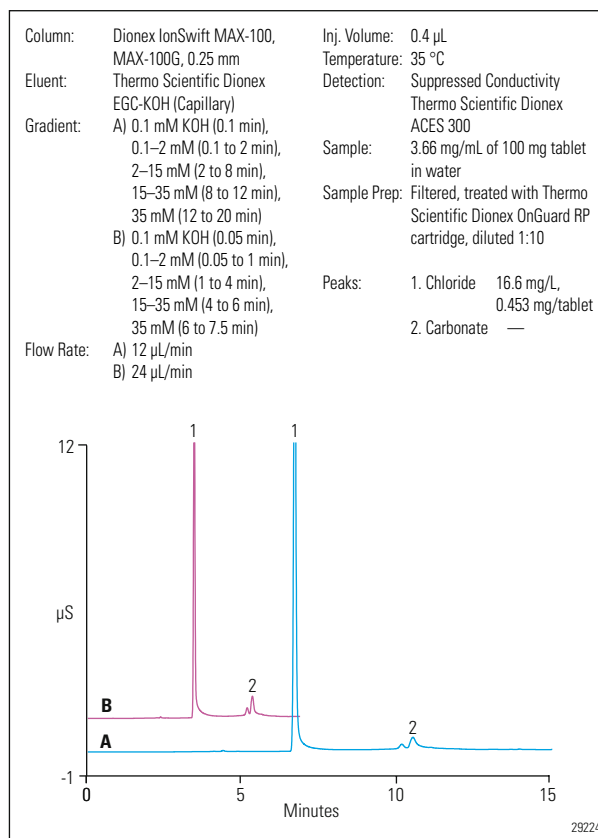


Figure 1. Capillary IC determination of the counterion in a drug used to treat type 2 diabetes.

Key Words

- Capillary IC
- High Pressure IC
- HPIC
- Dionex ICS-5000
- Dionex IonSwift MAX-100
- Type 2 Diabetes

Conditions

A Dionex ICS-5000 Capillary HPLC system, Thermo Scientific Dionex AS-AP Autosampler, and Thermo Scientific Dionex Chromleon Chromatography Data System software were used in this experiment. All experimental parameters are listed in Figure 1.

Sample Information and Preparation

Extract the counterion analyte by dissolving the diabetes treatment tablet in water at elevated temperature. After filtration, dilute the sample solution tenfold prior to analysis.

References

1. Thermo Fisher Scientific. *Quantification of Anions in Pharmaceuticals*, Application Note 116, LPN 0924. Sunnyvale, CA, 2007. <http://www.dionex.com/en-us/documents/lp-71572.html>
2. Wermuth, C.G.; Stahl, P.H. *Handbook of Pharmaceutical Salts: Properties, Selection and Use*, Wiley-VCH, Weinheim, Germany, 2002, pp 1–7.
3. Berge, S.M.; Bighley, L.M.; Monkhouse, D.C. *Pharmaceutical Salts*, *J. Pharm. Sci.* 1977, 66 (1), 1–19.

In addition to these offices, Thermo Fisher Scientific maintains a network of representative organizations throughout the world.

Dionex Products:
(408) 737-0700

**North America:
U.S./Canada**
(847) 295-7500

**South America:
Brazil**
(55) 11 3731 5140

**Europe:
Austria**
(43) 616 51 25

Benelux
(31) 20 683 9768
(32) 3 353 4294

Denmark
(45) 36 36 90 90

France
(33) 1 39 30 01 10

Germany
(49) 6126 991 0

Ireland
(353) 1 644 0064

Italy
(39) 02 51 62 1267

Sweden
(46) 8 473 3380

Switzerland
(41) 62 205 9966

United Kingdom
(44) 1276 691722

**Asia Pacific:
Australia**
(61) 2 9420 5233

China
(852) 2428 3282

India
(91) 22 2764 2735

Japan
(81) 6 6885 1213

Korea
(82) 2 2653 2580

Singapore
(65) 6289 1190

Taiwan
(886) 2 8751 6655

www.thermofisher.com

Legal Notices: ©2016 Thermo Fisher Scientific Inc. All rights reserved. All trademarks are the property of Thermo Fisher Scientific Inc. and its subsidiaries. This information is presented as an example of the capabilities of Thermo Fisher Scientific Inc. products. It is not intended to encourage use of these products in any manners that might infringe the intellectual property rights of others. Specifications, terms and pricing are subject to change. Not all products are available in all countries. Please consult your local sales representative for details.

LPN3058_E 08/16S