

Analysis of Per- and Polyfluoroalkyl Substances (PFAS) in Fish Fillet with LC-MS/MS

Nozomi Maeshima¹, Kota Ishioka¹, Toshiya Matsubara², Manami Kobayashi¹

1) SHIMADZU Corporation, Kawasaki, Japan; 2) Shimadzu Scientific Instruments, Columbia, MD



1. Introduction

Per- and Polyfluoroalkyl Substances (PFAS) is the collective name for a chemical group of organic fluorinated compounds, perfluorooctane sulfonate (PFOS) and perfluorooctanoic acid (PFOA) are representative compounds of PFAS. They have been used water repellents, surface treatment agents, fire extinguishers, and coatings. PFAS are persistent and bioaccumulative in the environment because of their stable structure, it is known that they are present in a wide range of environmental water and wildlife. Due to concerns about human exposure through diet, studies on the status of food contamination by PFAS are being conducted in various countries. We have examined a quantitative analysis method for thirty PFAS compounds in fish fillet samples.

2. Methods

2-1. Sample and equipment

Standard compounds were purchased from Wellington Laboratories. Fish fillet for sample was purchased from a local grocery store and homogenized using a freeze grinder FST-4000 (AiSTI SCIENCE). Quantification was performed with a triple quadrupole mass spectrometer LCMS-8060NX equipped with NexeraTM X3 UHPLC (Shimadzu Corporation, figure 1). The system configuration is shown below. To prevent contamination from an equipment, a delay column was added between a mixer and an autosampler.

Nexera X3 system

Column : Shim-pack ScepterTM C18-120 (100 mm x 2.1 mm I.D., 3 μ m)
 Delay column : Shim-pack Scepter C18-120 (50 mm x 2.1 mm I.D., 3 μ m)
 Mobile phase A : Acetonitrile/water = 5:95(v/v) with 2 mmol/L Ammonium acetate
 Mobile phase B : Acetonitrile
 Rinse : Methanol/water = 50:50(v/v)
 Flow rate : 0.3 mL/min (0.6 mL/min only between 10.01-12 min)
 Time program : B conc. 20% (0 min) \rightarrow 100% (10-12 min) \rightarrow 20% (12.01-15 min) The flow was introduced into the mass spectrometer between 1 to 9.6 min using a flow switching valve.
 Column temp. : 40 °C Injection vol. : 5 μ L



Figure 1. Nexera X3 and LCMS-8060NX

2-2. Extraction

The extraction procedure was performed with reference to the QuEChERS method. The flow is shown in Figure 2. A frozen and ground sample of 10 g was weighed and added with 10 mL of acetonitrile, then vigorously shaken for 1 minute. One packet of Q-sep QuEChERS extraction salt (Restek, P/N: 25849) was added and immediately shaken vigorously by hand for 1 minute. The mixture was centrifuged at 4,000 rpm at room temperature for 5 minutes, and the acetonitrile layer was collected. This acetonitrile layer was diluted 5 times with water to obtain the extraction solution.

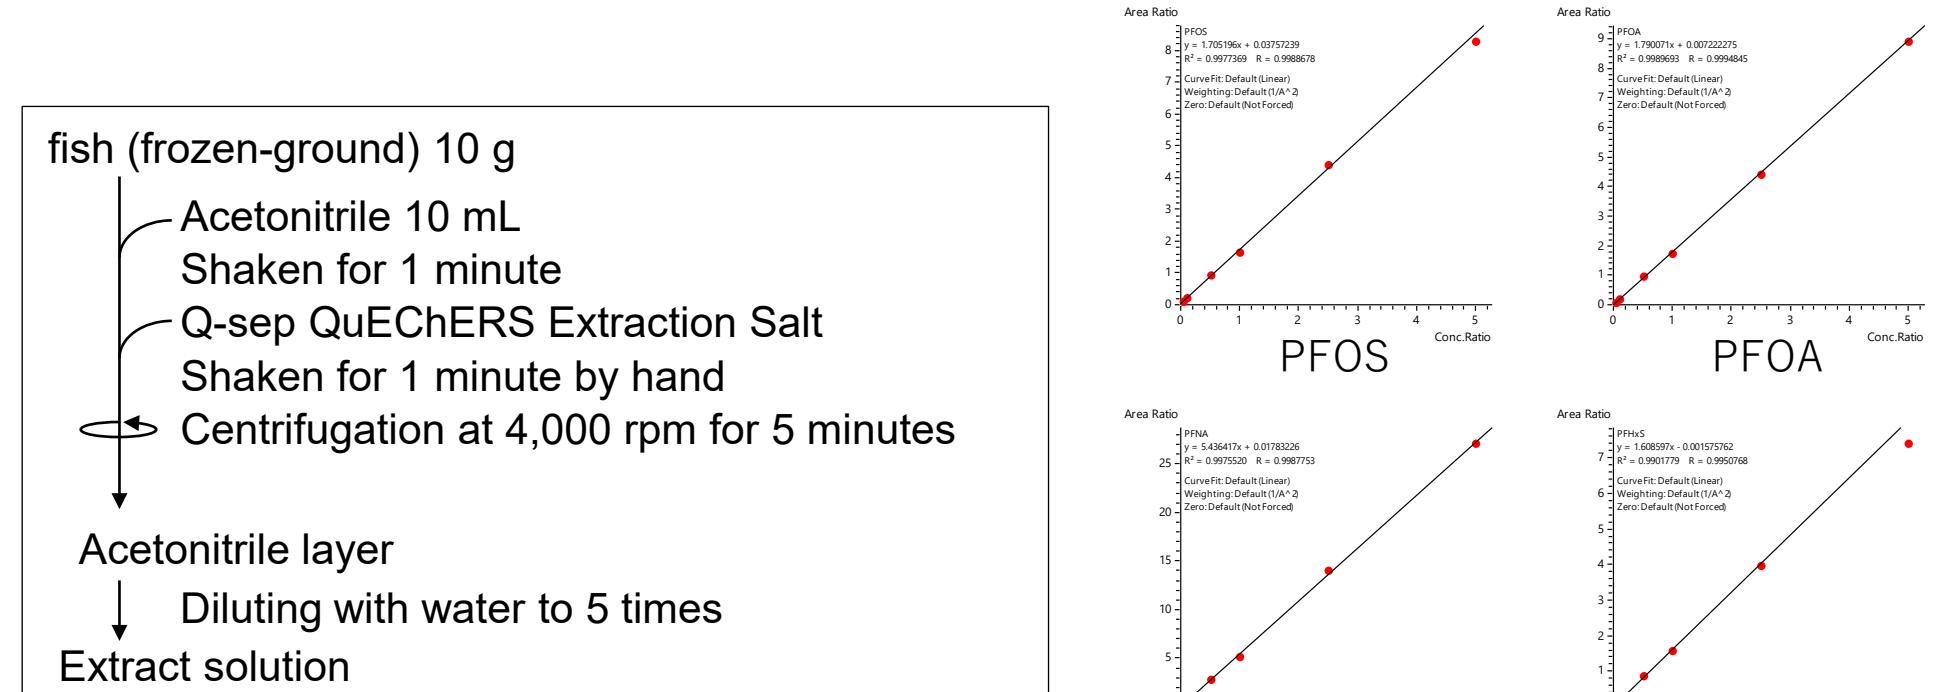


Figure 2. The extraction process

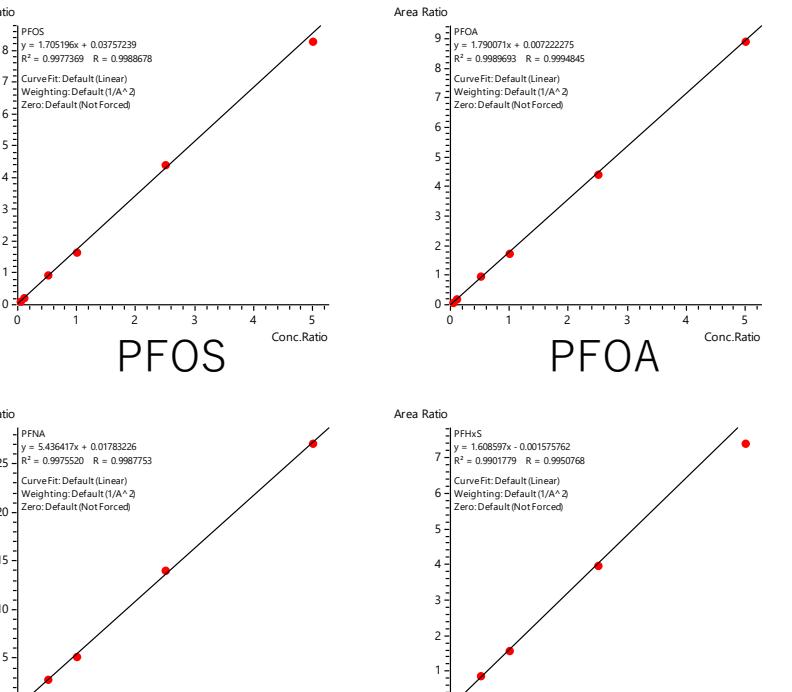


Figure 5. Calibration curves ranging from 0.05 - 5 μ g/kg (spiked conc.)

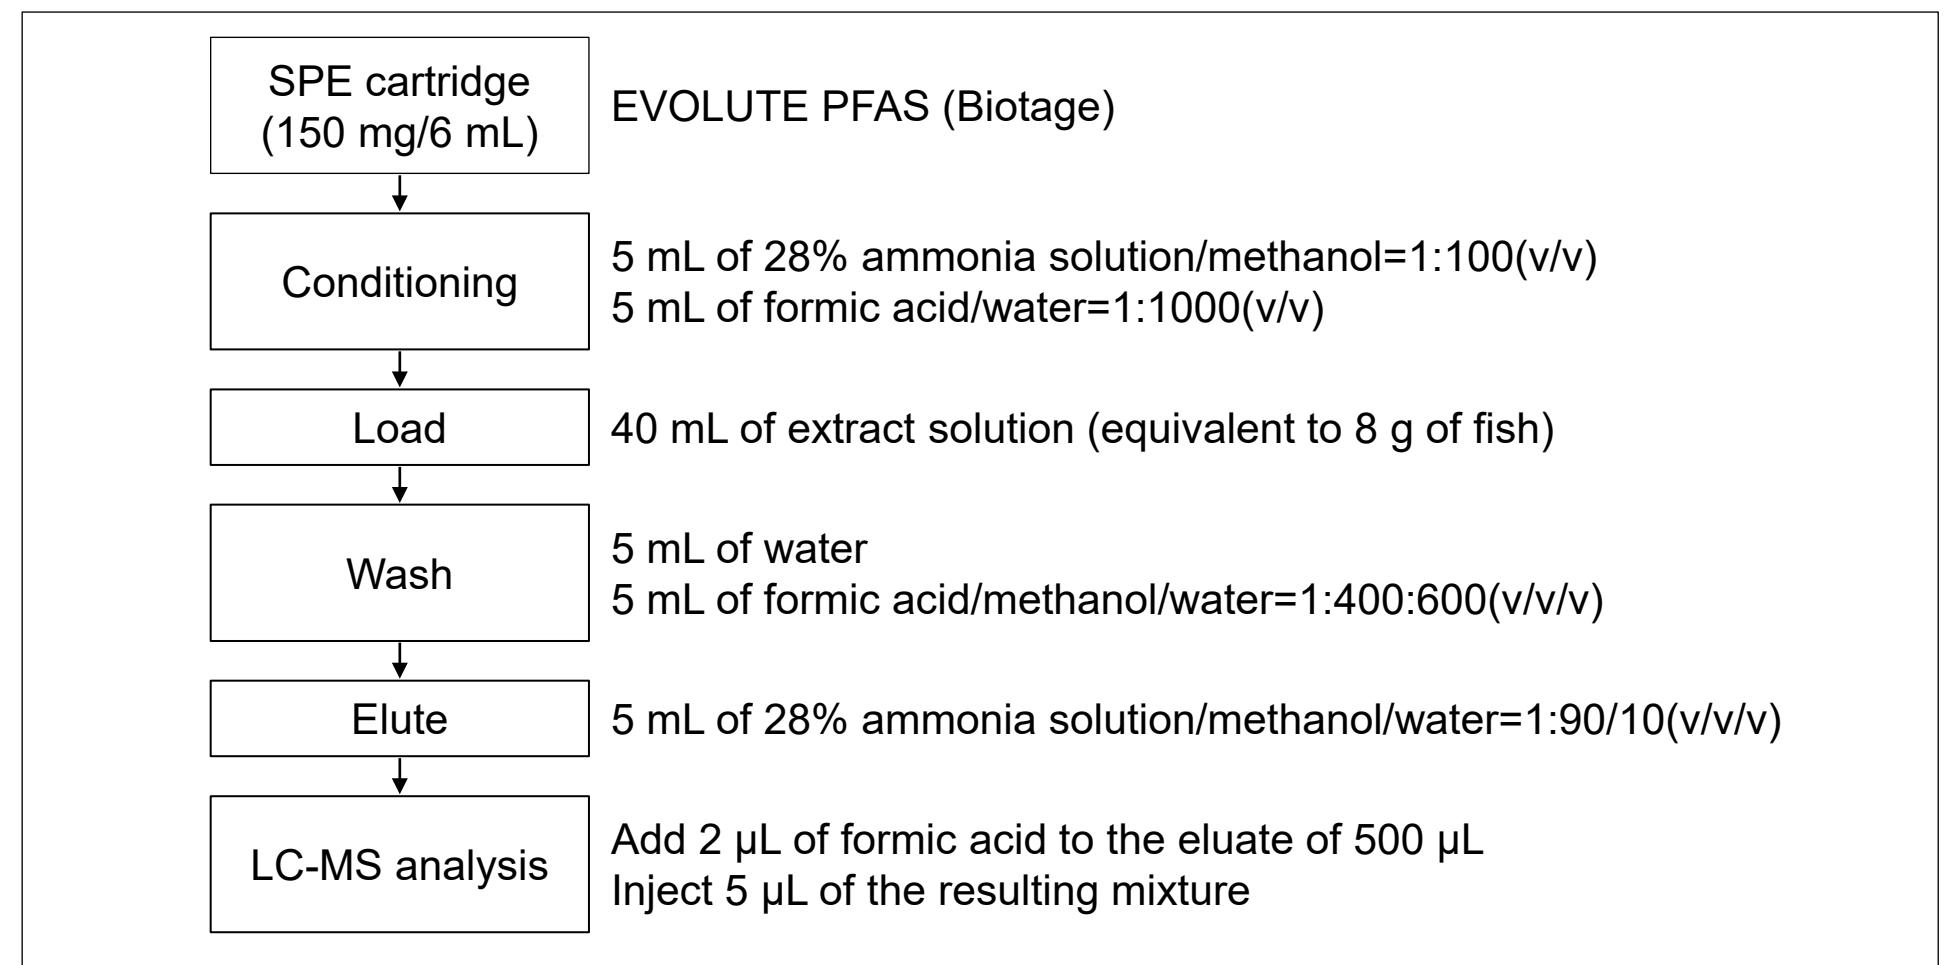


Figure 3. The purification process

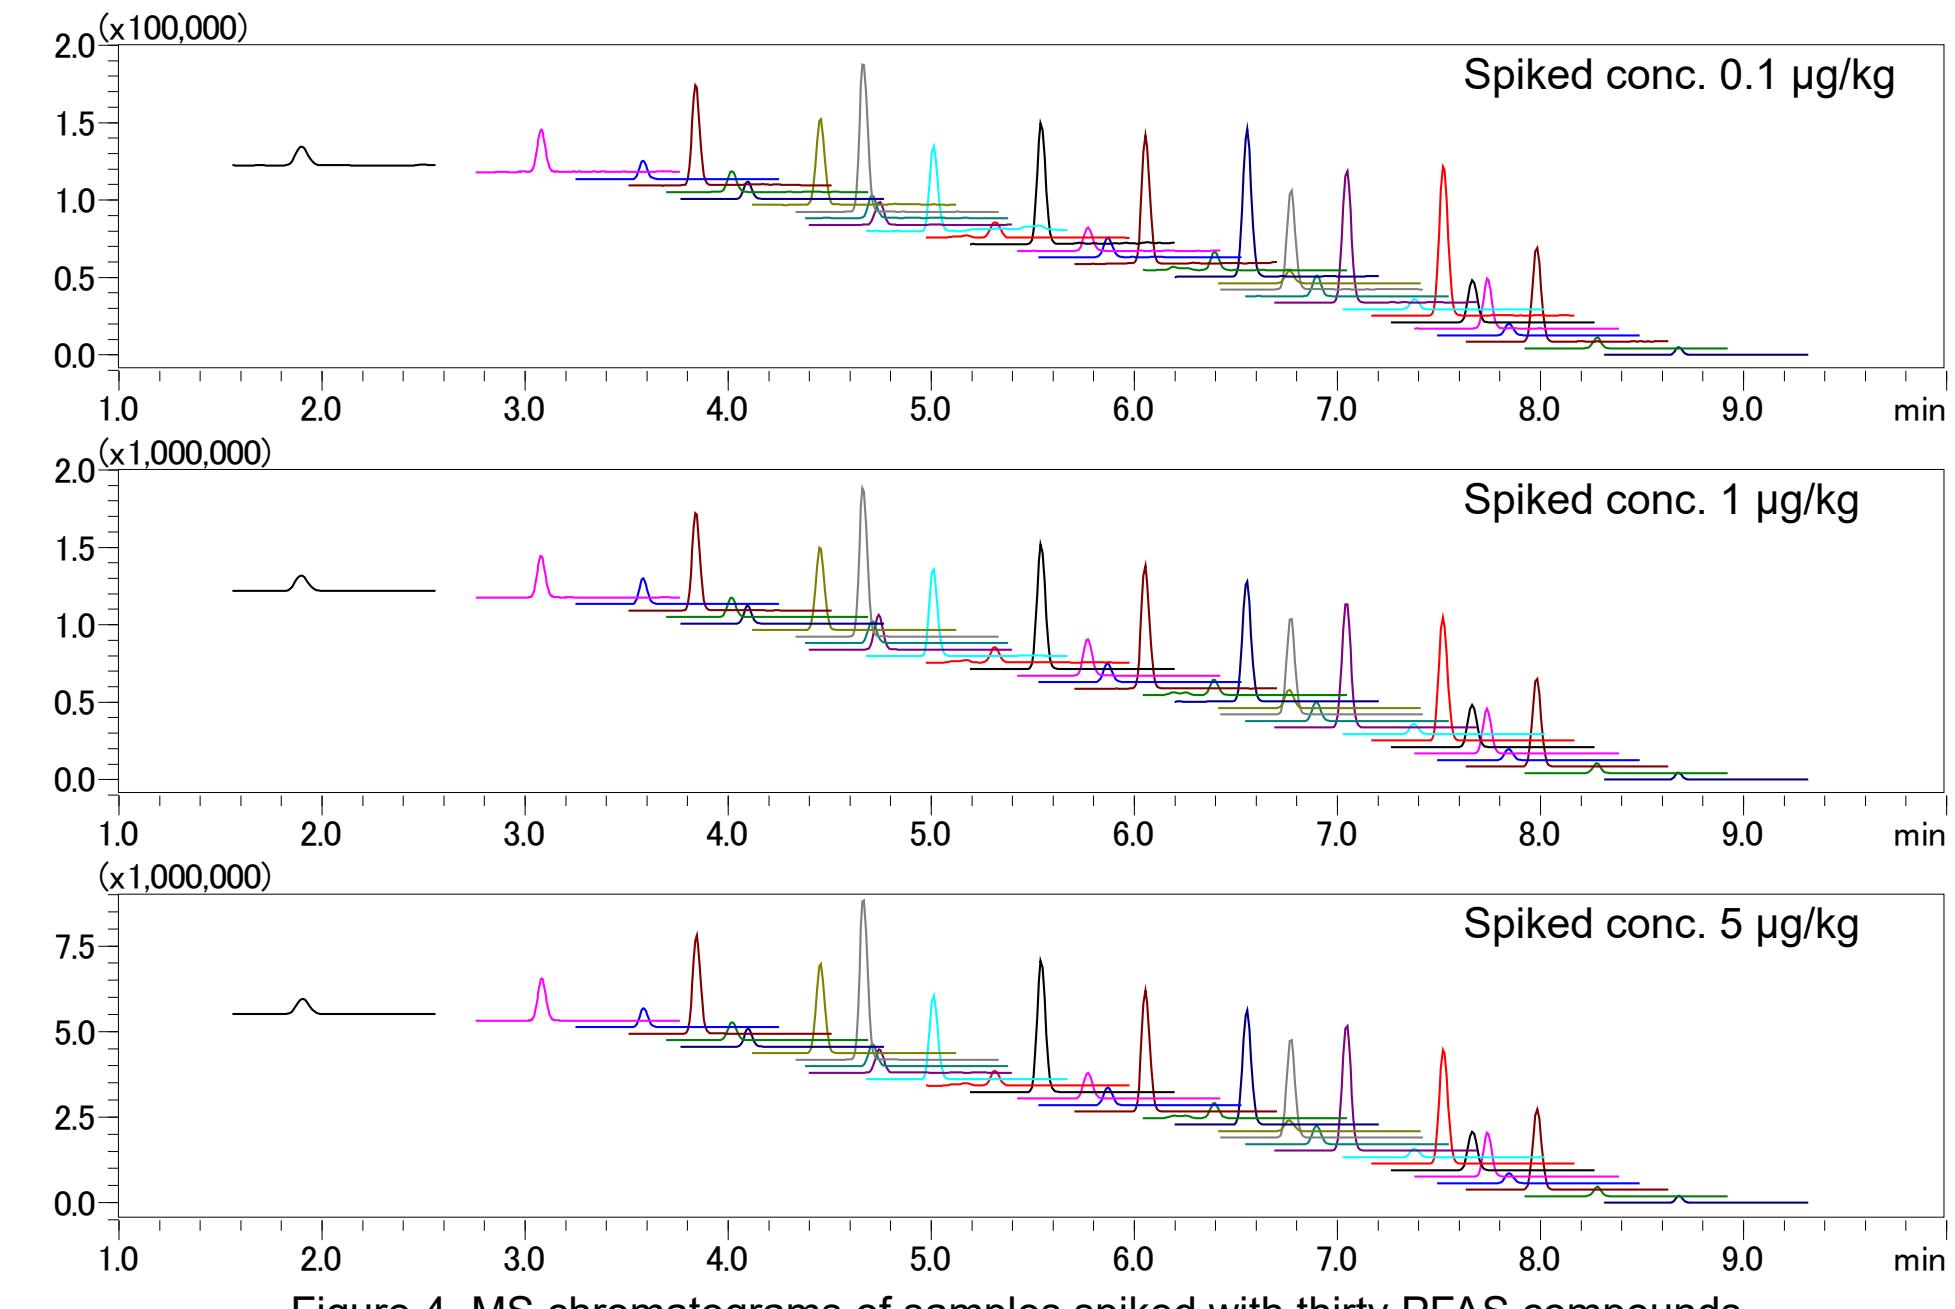


Figure 4. MS chromatograms of samples spiked with thirty PFAS compounds

3-2. Recovery rate test

Recovery tests were conducted at concentrations of 0.1, 1, and 5 μ g/kg to verify the recovery rates and repeatability. Preprocessing was performed in triplicate, and matrix-matched calibration curves were used for quantification. According to the requirements of the AOAC SMPR, PFOS, PFOA, PFNA, and PFHxS have a LOQ of 0.1 μ g/kg, a recovery rate of 80-120%, and a repeatability of less than 20%. Other PFAS compounds have a LOQ of 1.0 μ g/kg, a recovery rate of 65-135%, and a repeatability of 25%. For all compounds, the recovery rates were within 80-120% and the repeatability was below 20% at the spiked concentrations of 0.1, 1, and 5 μ g/kg.

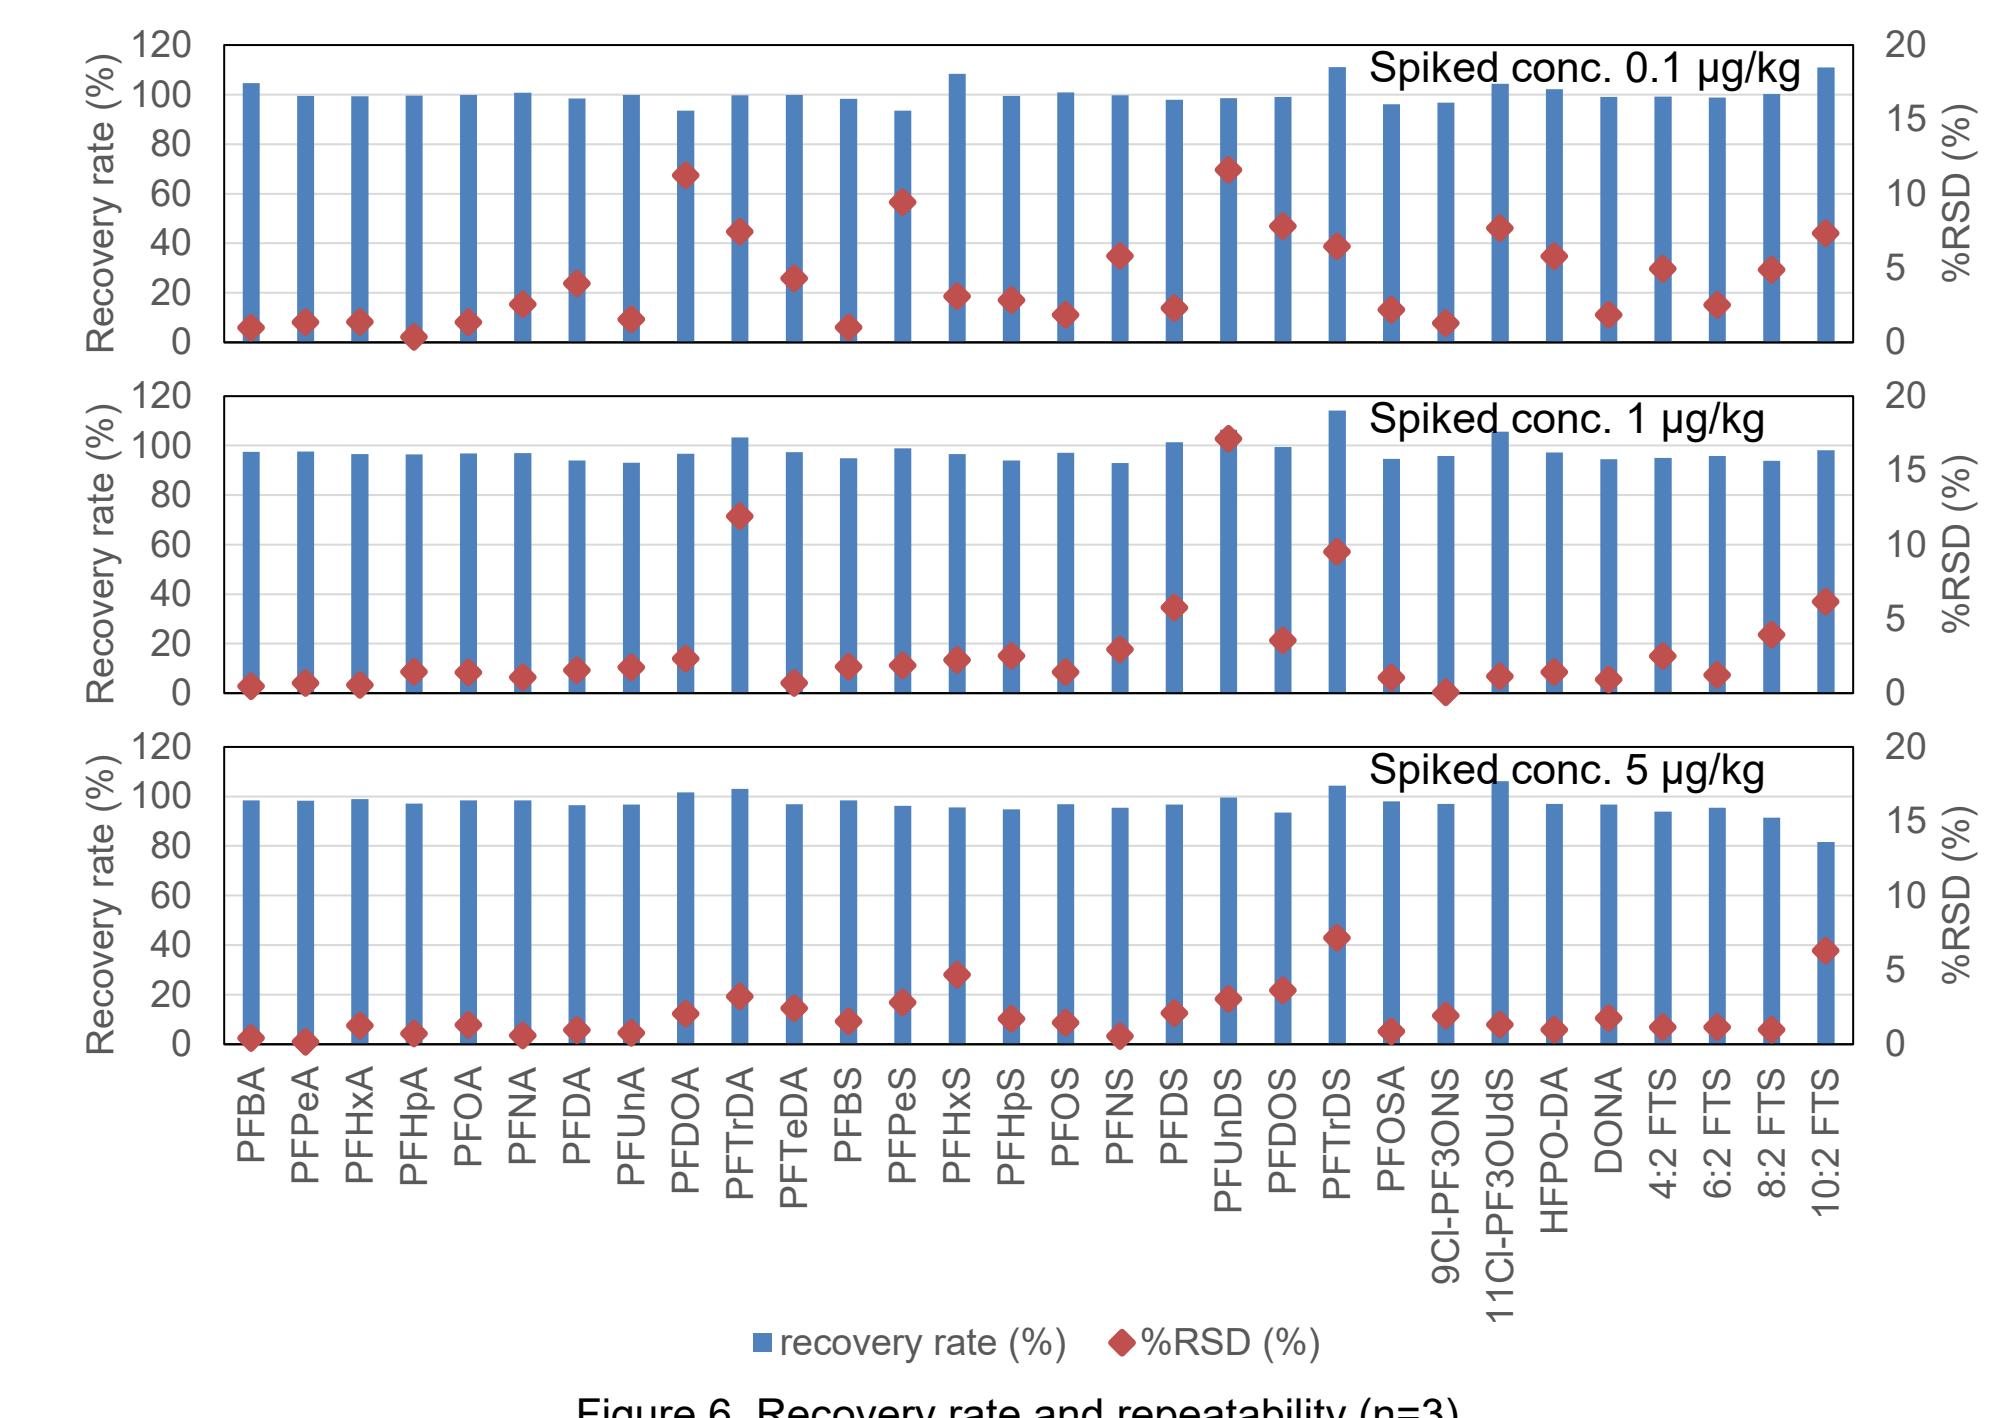


Figure 6. Recovery rate and repeatability (n=3)

3. Conclusions

- An LC-MS method for thirty PFAS within fifteen minutes analysis were created.
- The development of the pre-processing step, and a recovery test were conducted at 0.1, 1, and 5 μ g/kg, resulting in favorable results. Recovery rates within 80-120% and repeatability below 20% were achieved for all compounds.

References

- AOAC SMPR@2023.003