

# Keep Your Lab Flowing


With RM on Your Agilent 1100 & 1200 HPLC Systems

Routine maintenance (RM) reduces downtime and protects your valuable analytical data. Use this guide to keep your Agilent 1100 and 1200 HPLC Systems operating at their best—replace these crucial components at the recommended intervals and keep extras on hand.

Factors such as analytical conditions, mobile phases and additives, and sample matrices can affect maintenance frequency.

[LEARN MORE](#)

For helpful maintenance videos and tips, plus a full list of replacement parts, visit [www.restek.com](http://www.restek.com)

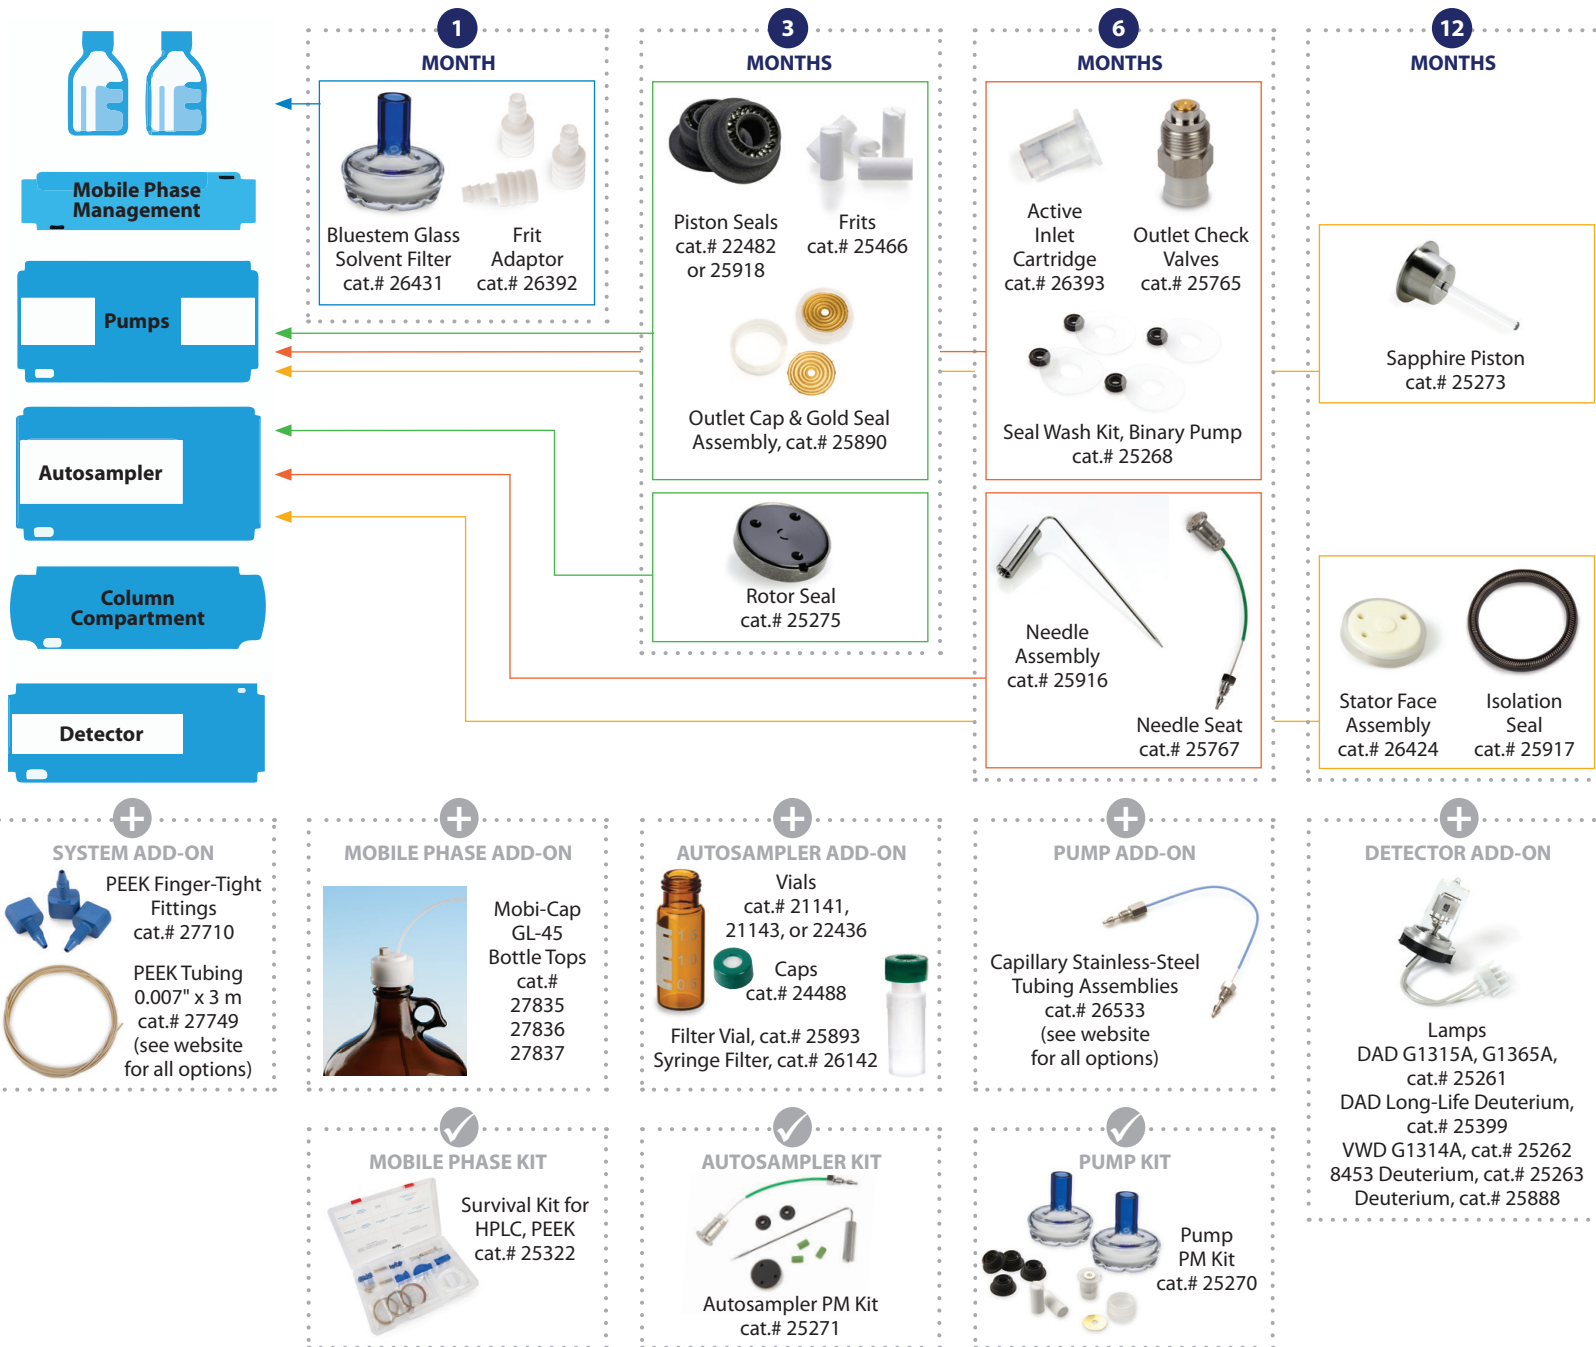

Questions about this or any other Restek product? Contact us or your local Restek representative ([www.restek.com/contact-us](http://www.restek.com/contact-us)).

Restek patents and trademarks are the property of Restek Corporation. (See [www.restek.com/Patents-Trademarks](http://www.restek.com/Patents-Trademarks) for full list.) Other trademarks in Restek literature or on its website are the property of their respective owners. Restek registered trademarks are registered in the U.S. and may also be registered in other countries.

© 2020 Restek Corporation. All rights reserved. Printed in the U.S.A.

GNOT3158A-UNV