


# InertSearch™ for GC

InertCap® Applications

## Application of the PCB out of the insulating oil after cleaning up Data No. GA013-0000

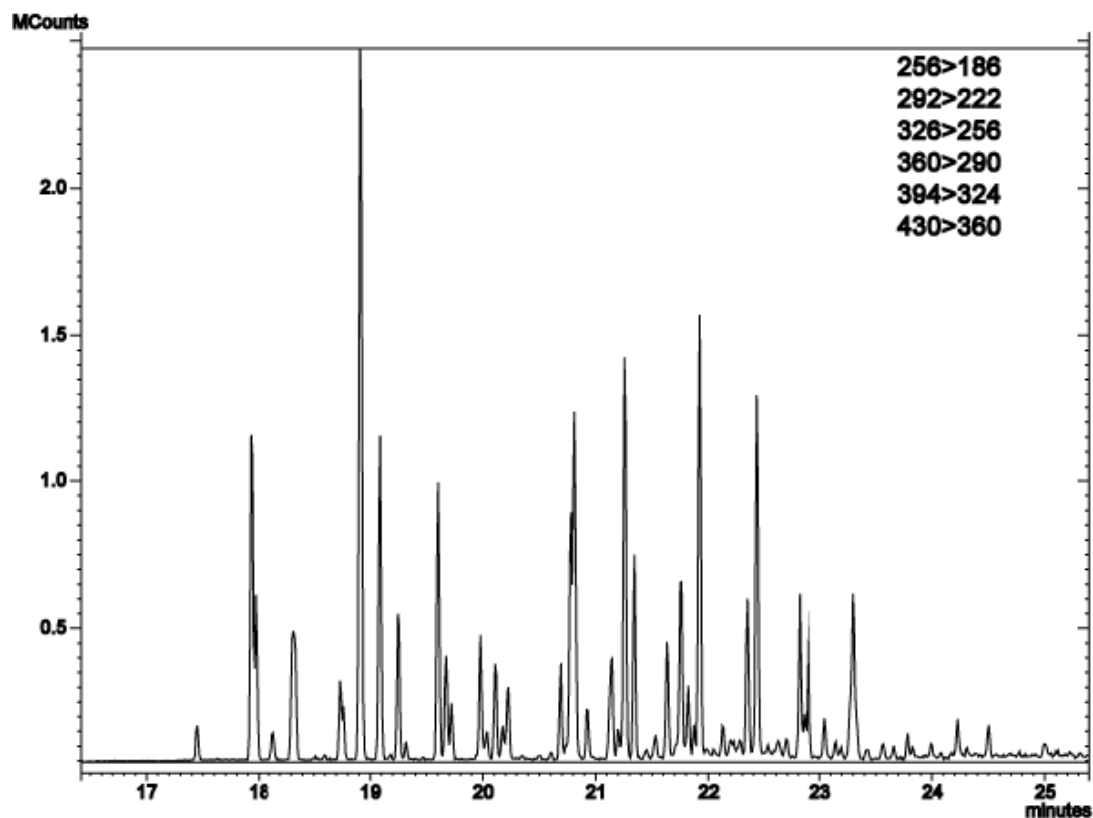

System : GC/MSMS PAC795 OPTIC3  
Column : InertCap 5MS/Sil  
0.25mmI.D.×30m df=0.25µm  
Column Temp. : 50°C (3min) → 15°C/min → 280°C  
Carrier Gas : He  
Injection : DMI 2µL  
60°C → 10°C/sec → 280°C  
Detection : MS/MS  
Collision Gas : Ar  
Sample : Insulating oil