


Organic Solvents

Data No. GA 283-0644

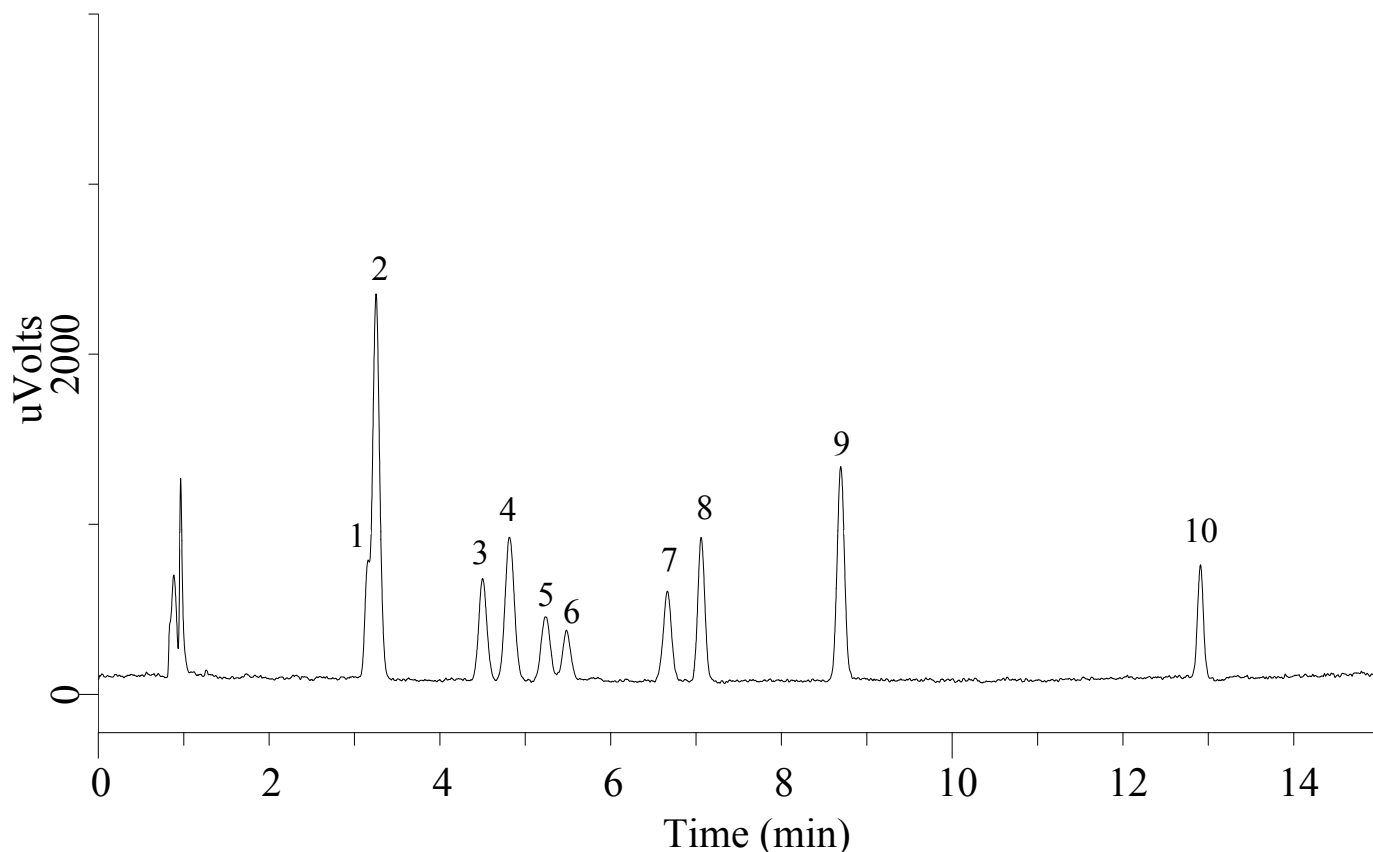

Conditions

System	: GC-FID	Analyte	: 1. Dichloromethane
Column	: InertCap WAX 0.53 mm I.D. x 30 m df = 1.0 µm		2. Benzene
Col. Cat. No.	: 1010-67445		3. Trichloroethylene
Col. Temp.	: 40 °C (5 min hold) - 5 °C/min - 180 °C		4. 4-Methyl-2-pentanone(MIBK)
Carrier Gas	: He 10 mL/min		5. Tetrachloroethylene
Injection	: Split flow 10 mL/min 220 °C		6. Chloroform
Detection	: FID Auto Range 220 °C		7. 1,4-Dioxane
Sample Size	: 2-4 ppm(V/V) in N ₂ 0.5 mL		8. 1,2-Dichloroethane
			9. Ethylbenzene
			10. Styrene